

# Page Proof Instructions and Queries


**Journal Title:** Prosthetics and Orthotics International

**Article Number:** 579319

Greetings, and thank you for publishing with SAGE. We have prepared this page proof for your review. Please respond to each of the below queries by digitally marking this PDF using Adobe Reader.

Click “Comment” in the upper right corner of Adobe Reader to access the mark-up tools as follows:

For textual edits, please use the “Annotations” tools. Please refrain from using the two tools crossed out below, as data loss can occur when using these tools.

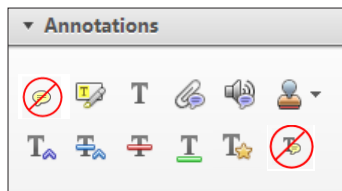


For formatting requests, questions, or other complicated changes, please insert a comment using “Drawing Markups.”



Detailed annotation guidelines can be viewed at: <http://www.sagepub.com/repository/binaries/pdfs/AnnotationGuidelines.pdf>  
 Adobe Reader can be downloaded (free) at: <http://www.adobe.com/products/reader.html>.

No.	Query
	Please note that this proof represents your final opportunity to review your article prior to publication, so please do send all of your changes now.
	Please review the entire document for typographical errors, mathematical errors and any other necessary corrections, and check headings, tables and figures.
	Please ensure that you have obtained and enclosed all necessary permissions for the reproduction of artistic works (e.g. illustrations, photographs, charts, maps, other visual material, etc.) not owned by yourself. Please refer to your publishing agreement for further information.
1	Please confirm that all author information, including names, affiliations, sequence and contact details, is correct.
2	Please check whether the manufacturer name ‘OMG / Vicon’ is correct as set.
3	Please check whether the location details inserted for the manufacturer ‘C-Motion, Inc.’ are correct.
4	Please check the sentence ‘The data were normalised ...’ for clarity.
5	Please note that ‘part 1’ has been changed to ‘session 1’ in the sentence ‘The results from session ...’. Please check.
6	Please check the sentence ‘Moreover, two outliers are revealed ...’ for clarity.
7	Please check the sentence ‘The application of the 3D cluster ...’ for clarity.
8	Please check the sentence ‘It can be clearly seen ...’ for clarity.
9	Please confirm that the author contribution, conflict of interest and funding statements are accurate.
10	Please note that some of the references have been renumbered to make their citations sequential in text. Please check.

# Multi-segment kinematic model to assess three-dimensional movement of the spine and back during gait

Prosthetics and Orthotics International  
1–12  
© The International Society for  
Prosthetics and Orthotics 2015  
Reprints and permissions:  
sagepub.co.uk/journalsPermissions.nav  
DOI: 10.1177/0309364615579319  
poi.sagepub.com  
The SAGE logo, consisting of a stylized 'S' inside a circle followed by the word 'SAGE'.

Robert Needham, Roozbeh Naemi, Aoife Healy and  
Nachiappan Chockalingam **[AQ: 1]**

## Abstract

**Background:** Relatively little is known about spine during gait compared to movement analysis of the lower extremities. The trunk is often regarded and analysed as a single rigid segment and there is a paucity of information on inter-segmental movement within the spine and its relationship to pelvis and lower limbs.

**Objectives:** To develop and validate a new multi-segment kinematic model to assess regional three-dimensional movement of the lumbar, lower thoracic and upper thoracic spine during gait.

**Study design:** Observational study.

**Methods:** The study was conducted in two parts: (1) to provide validation measures on the kinematic model built in commercially available software and (2) to apply the marker configuration to the spine at T3, T8 and L3 during gait analysis on 10 healthy male volunteers.

**Results:** Proposed model revealed excellent concurrent validation measures between an applied input angle to the recorded output angle from the kinematic model. A high reliability was observed during gait analysis, both during a single session and between sessions for all participants.

**Conclusion:** The thoracic region of the spine should not be modelled as a single rigid segment and the proposed three-dimensional cluster is reliable and repeatable to assess the inter-segmental movement of the spine.

## Clinical relevance

Reliable kinematic data can be collected using the three-dimensional cluster technique, thus, allowing researchers to accurately distinguish between movement patterns of healthy individuals to those with a clinical condition, and provide confidence in data acquisition during the monitoring process of an implemented rehabilitation intervention programme.

## Keywords

Spine kinematics, gait analysis, three-dimensional movement, spine model

Date received: 26 November 2014; accepted: 22 February 2015

## Background

Clinical conditions such as leg length discrepancy (LLD) can adversely affect movement of the spine and the coupling between the spine and pelvis during gait.<sup>1</sup> These changes in the coordination pattern between the pelvis and spine have been implicated as a biomechanical factor associated with the development of low back pain (LBP).<sup>2,3</sup> Thus, an understanding of spinal motion while walking in coordination with the lower limbs<sup>4,5</sup> will assist in the assessment and clinical management of individuals with spinal pathologies. Such knowledge could also be used to monitor an interventional strategy following the prescription of an ambulatory aid for the purpose of restoring normal gait patterns.

Marker-based motion capture systems are widely used in gait analysis laboratories, providing accurate kinematic measurements and a quantitative means of assessing gait impairment. Various kinematic models designed to assess pelvis and lower limb movement have been validated and are regularly implemented in external gait laboratories.<sup>6,7</sup>

---

Staffordshire University, Stoke-on-Trent, UK

### Corresponding author:

Nachiappan Chockalingam, Staffordshire University, Leek Road, Stoke-on-Trent ST4 2DF, UK.

Email: n.chockalingam@staffs.ac.uk

However, the examination of spine motion during gait has received little attention compared to movement analysis of the lower extremities.<sup>8–10</sup>

Kinematic modelling of the thorax and analysing movement of this segment relative to the pelvis normally consider the trunk as a rigid segment. While considered to be a suitable approach for clinical gait analysis,<sup>11</sup> a defined thorax segment has yet to be agreed upon in the scientific literature.<sup>11–14</sup> Furthermore, conventional gait models disregard movement in the lumbar region and are unable to provide information on the coordinated interaction between multiple segments of the spine. Recently, Leardini et al.<sup>11</sup> proposed a five-segment trunk model for gait analysis which included a segmental analysis of the lumbar spine. However, the inability to place markers on accessible anatomical landmarks limited the analysis of the lumbar segments to the sagittal and frontal plane.

Crosbie et al.<sup>15</sup> clearly demonstrated differences in ranges and patterns of motion for the lumbar, lower and upper thoracic spine during gait. Supportive evidence demonstrating inter-segmental movement of the spine is available in the literature.<sup>5,16</sup> Crosbie et al.<sup>15</sup> was also able to define the transverse plane in a coordinate system by placing additional markers on the surface of the back laterally to those attached to the spinous processes of the spine. Nevertheless, the independent movement between the markers placed on the skin, the back shape of an individual, and the influence of supporting musculature may subsequently contribute to segment angle calculations.

The attachment of a three-dimensional (3D) marker cluster onto the surface of the back and spine offers the advantage of allowing a cluster of markers to move relative to each other and allows for the tracking of movement in 3D. The coordinate system for the 3D cluster is based on the arrangement of the markers attached to the structure. Since these markers are also involved in tracking movement, it is only possible to analyse movement around the region of the spine where the 3D cluster is attached.

While it would seem that the 3D cluster technique is well documented in the literature, there are no standardised guidelines for the development, construction and application for the 3D cluster technique. Furthermore, the lack of detail in published studies on the materials and construction of the 3D cluster restricts the opportunity to investigate the external validity of this approach. Also, investigations often cite previously developed techniques but fail to provide a schematic of the replica 3D cluster to allow a comparison to the original.<sup>17</sup> To counteract the potential limitations of relatively larger structures,<sup>18</sup> Konz et al.<sup>5</sup> proposed the use of smaller 3D clusters that can be attached over the spinous processes using only double sided adhesive tape. However, reliability analysis and movement pattern waveforms of the

new proposed kinematic model were not documented. Consistent range of motion (ROM) values can be gained from utilising a 3D cluster when applied within the same gait laboratory.<sup>19–22</sup> However, there is limited evidence of time-series kinematic waveform analysis and an understanding of functional movement using the 3D cluster technique.

Therefore, the overall aim of this study is to develop a structured approach to assess the 3D kinematics of the lumbar spine. This approach will not only provide further clinically relevant inter-segmental movement of the thoracic region using 3D cluster which has not been reported but also highlight the importance of reporting global movement pattern data to explain relative movement.

## Methods


3D marker clusters adapted and based upon the design of previous investigations<sup>5,23,24</sup> were placed over the spinous processes of T3, T8 and L3 and were used to track movement in the upper thoracic (UT), lower thoracic (LT) and lumbar (L) region of the spine, respectively (Figure 1(a)). Each 3D cluster consisted of a silicone base plate and three non-collinear reflective markers attached to plastic tubing, fixed to the skin using double sided adhesive tape (Figure 1(b)). For reproducibility, the 3D clusters were constructed from components found in laboratories that use a optoelectronic motion capture system.<sup>25</sup>

### Coordinate systems

The global coordinate system (GCS) was defined with the X-axis corresponding to the anterior–posterior direction (positive X-direction indicated forward progression). The Y-axis was defined as medio-lateral perpendicular to the X-axis parallel to the ground (positive Y-direction pointing to the left). The Z-axis corresponded to the vertical direction (positive Z-direction pointing upwards).

The origin of the pelvis segment local coordinate system (LCS) was the mid-point between the two anterior–superior–iliac spine markers that defined the Y-axis. The X-axis was directed in an anterior direction perpendicular to the Y-axis from the mid-point of the anterior–superior–iliac spine and mid-point between the posterior–superior–iliac spine markers. The Z-axis was formed by the cross product of the X- and Y-axis.

The L, LT and UT LCS were defined using the three markers attached to each 3D cluster. The Y-axis was defined as a line passing through the two markers mounted on the lateral ends of the 3D cluster (positive direction to the left). The Z-axis was defined from the mid-point between the lateral markers on the 3D cluster to the vertical marker (positive direction upwards). The X-axis was the cross product of the Y- and Z-axis (positive direction forwards).

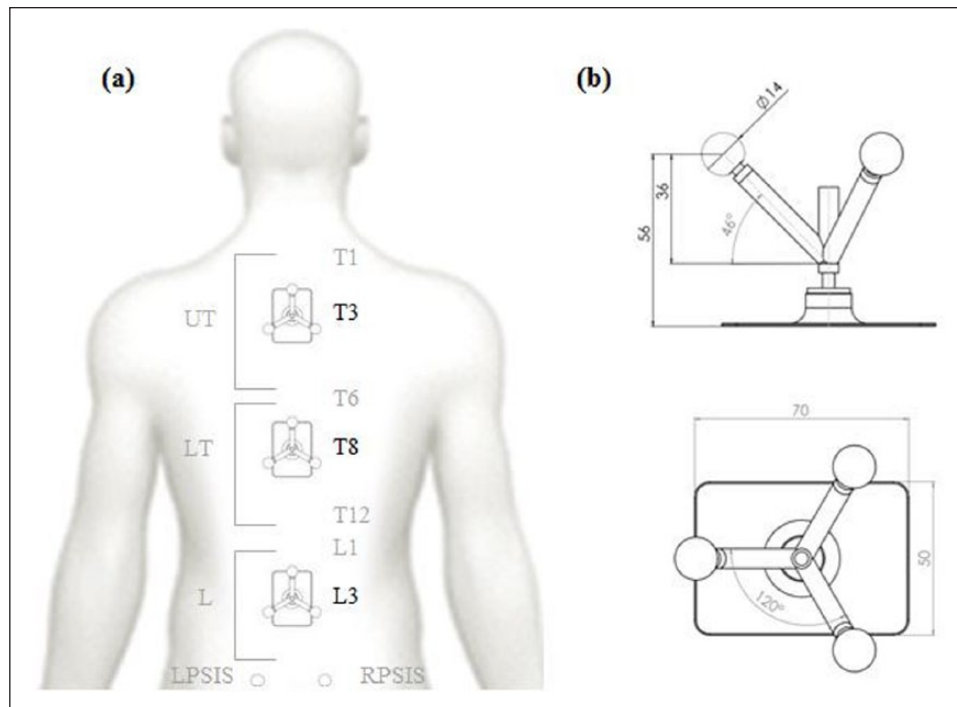

**Figure 1.** (a) Marker set configuration and (b) cluster rig dimensions (useless stated all measurements are in millimetres).

### Joint parameters

3D angles were calculated with respect to the normal standing position of the participant. Rotations about the GCS and LCS were based on the right-hand rule convention. Angular kinematic data were computed by measuring the relative movements between the 3D clusters and pelvis: UT relative to LT, LT relative to L and L relative to the pelvis. In addition to the pelvis, movement data from the 3D clusters was also reported relative to the GCS. Cardan angles were calculated using the YXZ (anterior–posterior tilt/flexion–extension, obliquity/lateral flexion and axial rotation).<sup>26</sup>

### Instrumentation and software

An eight camera motion capture system (OMG / Vicon, Oxford, UK) was used to record 3D coordinate data at 100 frames/s. [AQ: 2] The capture volume was defined with dimensions of  $2.5 \times 2 \times 6$  m. The kinematic spine model was developed in Visual3D (C-Motion, Inc., Germantown, MD, USA) and the marker coordinate data were processed using a low-pass Butterworth filter with a cut-off frequency of 6 Hz.<sup>27</sup> [AQ: 3]

### Experimental procedures – kinematic model accuracy and precision


To validate the proposed kinematic spine model created in Visual3D, the marker configuration was applied to a mechanical frame that represented a replica of a human spine, which had the capability of moving in all three planes

of motion (Figure 2(a)). To test the accuracy and precision of the generated output from Visual3D software, angle data were compared against 10 known static reference positions ( $0^\circ$ ,  $2^\circ$ ,  $4^\circ$ ,  $6^\circ$ ,  $8^\circ$ ,  $10^\circ$ ,  $12^\circ$ ,  $15^\circ$ ,  $30^\circ$  and  $45^\circ$ ). Predetermined reference positions were also chosen to test angle estimation from dynamic trials (tracking movement from  $0^\circ$  to  $30^\circ$ ).

A flexible electro-goniometer (FEG) and a torsio-meter (TM) (model SG150b and Q150, respectively; Biometrics Ltd, Gwent, UK) were attached to the mechanical frame on separate occasions (Figure 2(b)). The FEG and TM were the chosen criterion reference from which static and dynamic reference positions were determined. The validation of the FEG has been reported elsewhere.<sup>28</sup> The FEG and TM both consist of two lightweight plastic end-blocks at either end of a spring containing a strain gauge mechanism. The end-blocks of the FEG and TM were attached at proximal and distal locations to the joint centre on the mechanical frame. The LCS for each 3D cluster was constructed in the same way within Visual3D; therefore, only the UT 3D cluster was chosen during the kinematic model validation procedures. Relevant hardware (Biometrics Data-link) and associated software was synchronised with the motion capture system and recorded five 5 s trials for flexion and extension (FEG), left and right lateral flexion (FEG) and axial rotation (TM) movements. Angle outputs were recorded to two decimal places.

### 3D cluster – application during gait

A total of 10 healthy males, with a mean age of 22.4 ( $\pm 2.46$ ) years, height of 180.3 ( $\pm 7.18$ ) cm and mass of

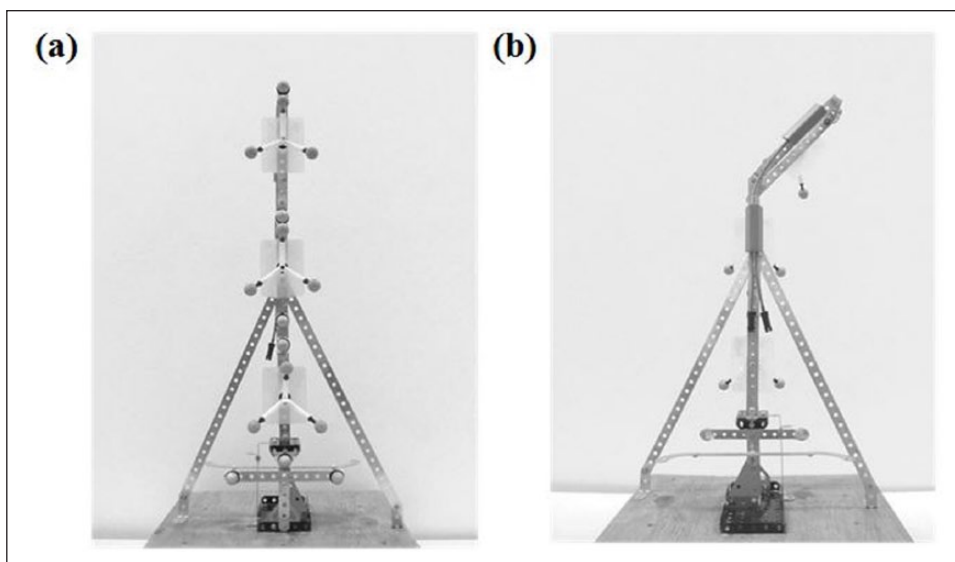

**Figure 2.** (a) Posterior view of the marker set configuration attached to the mechanical frame and (b) anterior view of the flexible electro-goniometer (FEG) attached to the mechanical frame.

74.97 ( $\pm 11.02$ ) kg, with no history of musculoskeletal impairments participated in the study. Ethical approval was sought and received from the University Committee and all participants provided an informed consent.

### Procedure for data collection

Participants were required to walk barefoot at a preferred walking speed (PWS). Wireless timing gates (Brower Timing Systems, Draper, UT, USA) were used during data collection to ensure PWS was achieved. A motion capture system was used to record kinematic data over five trials along with two AMTI-OR6 force platforms (Advanced Mechanical Technology, Inc. (AMTI), Watertown, MA, USA) to assist in the identification of gait events (initial contact and toe off). This procedure was repeated 1 week later to examine test–retest reliability; walking speed was matched to session 1.

## Results

### Kinematic model accuracy and precision

Linear regression analysis was used to produce the best-fit line through the data relating the applied input angle (TM/FEG) to the output angle from Visual3D software (kinematic model) (Figure 3). Standard error of the measurement (SEM) (range:  $0.17^{\circ}$ – $0.35^{\circ}$ ), 95% confidence limits (range:  $0.11^{\circ}$ – $0.72^{\circ}$ ) and coefficient of determination ( $R^2$ ) (0.99) values revealed excellent within and between session validity measures for the static reference trials (Figure 3). Coefficient of multiple correlation analysis for the dynamic trials revealed excellent inter-validity measures (0.91–0.95) for left and right axial rotation.


### 3D cluster – application during gait

The data were normalised and time scaled to 100% of the gait cycle, from right initial contact to right initial contact. **[AQ: 4]** To assist in the interpretation of kinematic waveforms, the phases of gait as defined by Perry and Burnfield<sup>29</sup> were included (IC: initial contact; LR: loading response; MS: mid-stance; PS: pre-swing; swing phase). Table 1 summarises temporal and distance parameters from sessions 1 and 2. Figure 4 provides time-series kinematic waveforms along with the mean difference between sessions 1 and 2 at each point of the gait cycle. Table 2(a to c) represents mean ROM and standard deviation values for the group and individual participants, respectively, for L, LT and UT region during gait. Table 2(d to f) also provides intra-/inter-participant repeatability measures, assessed by the average standard deviation (AvgSD), representative of each standard deviation value for each data point over the gait cycle.<sup>11</sup>

## Discussion

### Kinematic model accuracy and precision

Adopting a similar approach to a previous study<sup>30</sup> for the purpose of validating a kinematic model, Konz et al.<sup>5</sup> built a mechanical frame that replicated the spine and using a manual goniometer, regions of the mechanical spine were positioned at  $30^{\circ}$  increments to compare an applied angle to an angle output generated from a kinematic model. The authors reported a measurement error of  $2^{\circ}$ – $5^{\circ}$  between predetermined angles and angles generated by the kinematic model; therefore, the accuracy and precision of this technique is questionable. Also, investigating increments

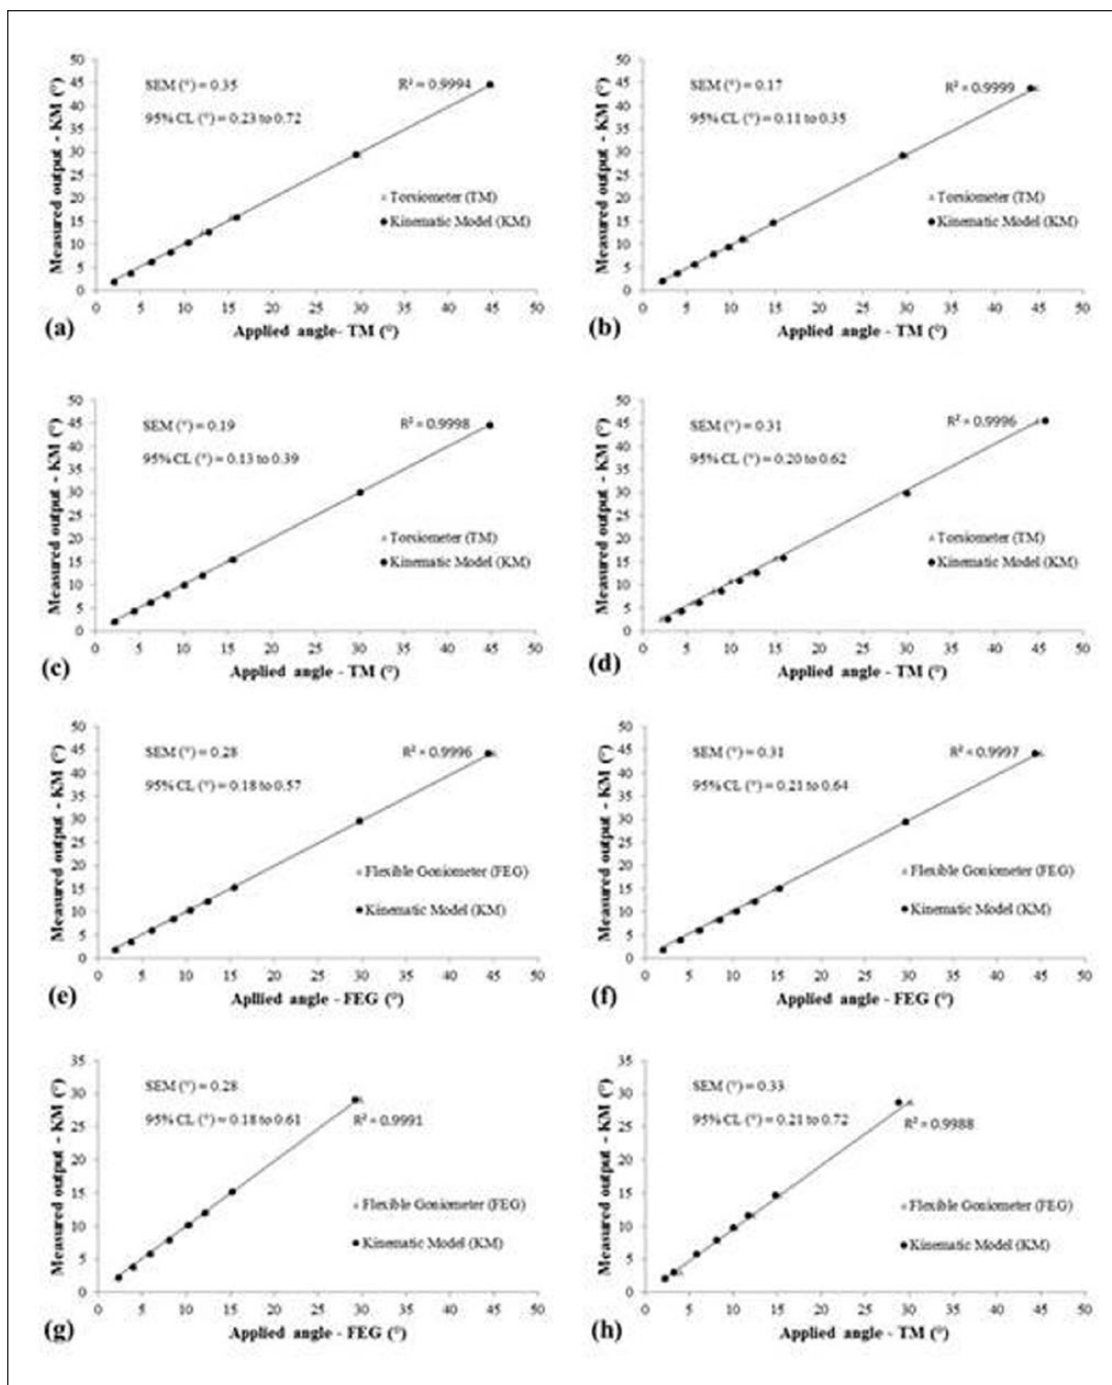


**Figure 3.** Relationship between the applied angle (TM/FEG) and the measured output (KM) for axial rotation (session 1 – (a) right and (b) left; session 2 – (c) right and (d) left), lateral flexion (session 1 – (e) right and (f) left) and flexion–extension (session 1 – (g) right and (h) left).

of 30° is not validating the angles that are experienced during gait. Nevertheless, thoracic and lumbar segment ROM values during gait cited by Konz et al.<sup>5</sup> were found to be consistent with the current literature. The TM and FEG employed in this study offer an alternative approach, allowing data to be analysed to less than a degree, which

can be comparable to the angle output from the kinematic model constructed in Visual3D software (values reported to two decimal places). In addition, the TM and FEG not only permit investigation of static trials but also allow for the assessment of dynamic movement. With a reported accuracy of  $\pm 1^\circ$ ,<sup>28</sup> the results of this study show the TM

**Table 1.** Temporal and distance parameters for session 1 (S1) and session 2 (S2) providing mean and standard deviation ( $\pm$ SD) values for each participant (P1–P10) and over the 10 participants.

Participant	Speed (m/s)		Stride length (m)				Cadence (steps/min)				Cycle time (s)				Stance time (s)				Swing time (s)			
	S2		S1		S2		S1		S2		S1		S2		S1		S2		S1		S2	
	Mean	SD	Mean	SD	Mean	SD	Mean	SD	Mean	SD	Mean	SD	Mean	SD	Mean	SD	Mean	SD	Mean	SD	Mean	SD
P1	1.60	1.55	1.62	0.03	1.54	0.03	117.00	4.77	119.00	4.66	1.00	0.03	1.00	0.02	0.57	0.02	0.56	0.01	0.43	0.01	0.44	0.01
P2	1.42	1.32	1.58	0.07	1.48	0.07	109.00	3.56	108.00	1.65	1.12	0.02	1.12	0.02	0.65	0.01	0.66	0.02	0.48	0.01	0.46	0.01
P3	1.34	1.38	1.41	0.04	1.42	0.04	115.00	4.34	116.00	3.14	1.06	0.02	1.03	0.03	0.63	0.01	0.56	0.03	0.44	0.01	0.46	0.03
P4	1.21	1.18	1.47	0.02	1.39	0.04	99.00	3.34	100.00	2.01	1.22	0.03	1.17	0.02	0.72	0.02	0.70	0.05	0.49	0.02	0.49	0.04
P5	1.47	1.49	1.60	0.02	1.61	0.03	111.00	2.84	111.00	2.88	1.09	0.04	1.07	0.01	0.63	0.03	0.62	0.01	0.45	0.02	0.45	0.01
P6	1.30	1.20	1.37	0.02	1.26	0.02	113.00	3.52	117.00	2.09	1.05	0.02	1.05	0.02	0.63	0.01	0.63	0.01	0.42	0.02	0.42	0.01
P7	1.21	1.29	1.41	0.03	1.42	0.03	105.00	2.94	108.00	3.54	1.18	0.01	1.09	0.03	0.71	0.01	0.67	0.02	0.47	0.02	0.43	0.01
P8	1.22	1.26	1.39	0.02	1.39	0.05	107.00	3.23	112.00	1.85	1.13	0.02	1.11	0.01	0.67	0.01	0.65	0.01	0.46	0.01	0.45	0.02
P9	1.09	1.07	1.26	0.06	1.18	0.04	108.00	5.25	111.00	2.57	1.16	0.06	1.10	0.01	0.70	0.04	0.68	0.01	0.46	0.02	0.42	0.01
P10	1.26	1.33	1.38	0.04	1.42	0.06	110.00	3.77	112.00	4.28	1.10	0.03	1.06	0.05	0.65	0.01	0.62	0.02	0.45	0.02	0.44	0.02
Group	1.31	1.31	1.45		1.41		109.40		111.40		1.11		1.08		0.66		0.64		0.46		0.45	
SD	0.15	0.14	0.12		0.12		5.17		5.42		0.07		0.05		0.05		0.05		0.02		0.02	

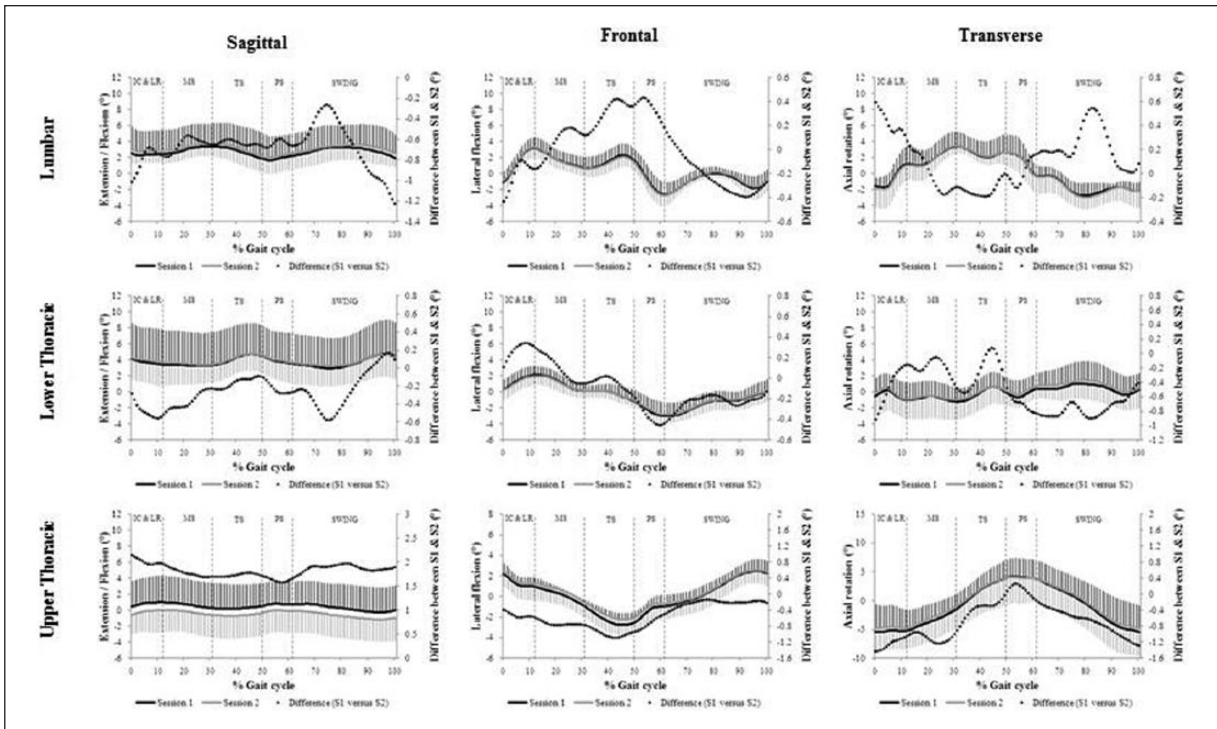

**Figure 4.** Time-series kinematic waveform data (reference to right vertical axis) for the lumbar segment, lower thoracic segment and upper thoracic segment in the sagittal, frontal and transverse plane represented over 10 participants for session 1 (black solid line) and session 2 (grey solid line).

Mean difference between sessions 1 and 2 at each time frame during the gait is presented (black dot).

and FEG to be an appropriate measure for concurrent validity. The results from session 1 (Figure 3) highlight the accuracy and reliability limits of the proposed kinematic model of this study and are in agreement with previous investigations.<sup>20,31</sup> [AQ: 5]

### 3D cluster – application during gait

With the objective to contribute further knowledge and understanding to the practicality and reliability of using a 3D cluster configuration, this study proposed a new kinematic model to measure 3D movement during gait in the region of T3, T8 and L3. The new multi-segment kinematic spine model presented in this study demonstrated high intra-subject repeatability (Table 2), and although there is noticeable variability in ROM values between participants, it is apparent that participant-specific movements can be tracked reliably between testing session.<sup>11</sup> Differences in temporal and distance parameters (Table 1) between participants combined with a small sample size could attribute to the high inter-participant standard deviation values for several ROM values (Table 2). Consistent kinematic waveforms presenting mean data from 10 participants and small mean difference values (Figure 4) along with comparable ROM values for each participant (Table 2) further demonstrated high reliability between sessions 1 and 2. Moreover, two outliers are

revealed in the analysis of the UT segment in the transverse plane (Figure 5(a)): a large ROM exhibited by one participant (black line) and an inappropriate placement of the rig on another participant (black dashed line). [AQ: 6]

Since this is the first study to report inter-segmental relative rotations of the thoracic spine using a 3D cluster technique, comparisons to previous published literature are not possible. The application of the 3D cluster to understand 3D lumbar motion on the other hand has received considerable attention. Table 3 allows for a comparison of ROM between values available in the published literature to those presented in this study. However, caution is warranted when comparing angle data due to the differences between studies in regard to the construction and application of the 3D cluster. The application of the 3D cluster over L3 was an approach taken by this study and that of Konz et al.<sup>5</sup> While contrasting ROM values exist; Konz et al.<sup>5</sup> did not report relative or global kinematic time-series information on movement patterns for the L3 region of the spine. [AQ: 7] Furthermore, comparative ROM values between this study and those from a study that used bone pins are noted in the sagittal and frontal plane.<sup>32</sup> In this study, similar ROM values were obtained between sessions 1 and 2. These findings support earlier work<sup>19–22</sup> by demonstrating the capability of the 3D cluster to gather reliable kinematic data when applied in the same



**Table 2.** Mean range of motion (ROM) and standard deviation (SD) values for the lumbar, lower and upper thoracic segment in the (a) sagittal, (b) frontal and (c) transverse plane over 10 participants during gait for sessions 1 and 2. Individual participant (P1–P10) and group average standard deviation values (AvgSD) representing the mean standard deviation of each data point over the gait cycle in the (d) sagittal, (e) frontal and (f) transverse plane for the lumbar, lower and upper thoracic segment for sessions 1 and 2.

Participant	(a) Sagittal											
	Lumbar						Upper thoracic					
	S1			S2			S1			S2		
	Mean	ROM	SD	Mean	ROM	SD	Mean	ROM	SD	Mean	ROM	SD
P1	2.90	1.82	0.49	4.64	0.88	3.83	0.64	2.07	0.77	1.94	0.62	
P2	4.16	4.05	0.77	3.34	0.81	3.34	0.78	2.26	0.32	2.54	0.48	
P3	4.01	0.79	3.02	2.02	0.66	3.17	0.16	1.45	0.21	2.00	0.22	
P4	2.82	0.17	3.33	5.70	1.24	4.94	0.36	3.68	0.78	3.49	0.92	
P5	3.97	0.81	3.66	3.09	0.56	2.91	0.46	3.19	0.45	2.85	0.62	
P6	3.49	1.02	3.17	7.54	0.86	4.54	1.06	2.78	0.26	1.85	0.25	
P7	2.99	0.99	2.32	2.87	0.95	2.38	0.72	1.55	0.48	2.39	0.29	
P8	2.62	0.53	2.21	2.13	0.29	2.18	0.41	1.21	0.10	1.81	0.23	
P9	2.76	0.60	2.48	3.34	0.99	2.21	0.18	1.40	0.42	1.53	0.26	
P10	2.51	0.30	4.24	2.72	0.44	2.84	0.67	2.47	0.68	3.50	1.30	
Group	3.22	0.63	3.03	3.74	1.74	3.23	0.95	2.21	0.83	2.39	0.70	

Participant	(b) Frontal											
	Lumbar						Upper thoracic					
	S1			S2			S1			S2		
	Mean	ROM	SD	Mean	ROM	SD	Mean	ROM	SD	Mean	ROM	SD
P1	9.05	1.12	8.63	0.53	5.72	0.77	5.36	0.41	8.50	0.71	7.08	0.64
P2	7.18	1.44	7.78	0.90	3.16	0.70	2.61	0.52	8.71	1.23	7.09	0.72
P3	7.78	0.21	5.99	0.63	5.20	0.24	4.79	0.24	4.04	0.29	3.30	0.30
P4	6.17	0.64	7.25	0.88	11.44	0.94	8.33	0.69	5.09	0.25	5.38	0.94
P5	9.26	0.57	9.50	0.28	6.64	0.43	5.30	0.63	6.00	1.23	4.05	0.18
P6	7.14	0.44	5.47	0.61	3.38	0.34	3.31	1.20	6.92	0.57	5.66	0.96
P7	5.43	0.74	6.52	0.65	5.14	0.53	4.60	0.64	3.04	0.45	4.17	0.53
P8	3.52	0.43	4.71	0.04	5.00	0.60	5.00	0.38	4.23	0.70	3.75	0.54
P9	2.85	0.51	2.17	0.30	6.47	0.73	4.38	0.20	4.04	0.42	3.51	0.79
P10	6.66	0.58	8.32	0.50	3.24	0.54	4.45	0.60	5.48	0.53	3.91	0.57
Group	6.50	2.11	6.63	2.16	5.54	2.43	4.81	1.50	5.60	1.93	4.79	1.43

Participant	(c) Transverse											
	Lumbar						Upper thoracic					
	S1			S2			S1			S2		
	Mean	ROM	SD	Mean	ROM	SD	Mean	ROM	SD	Mean	ROM	SD
P1	0.55	0.38	0.12	0.12	0.13	0.07	0.15	0.12	0.12	0.12	0.15	
P2	0.22	0.17	0.13	0.11	0.18	0.18	0.18	0.11	0.18	0.16	0.15	
P3	0.10	0.17	0.11	0.23	0.23	0.18	0.11	0.11	0.08	0.08	0.19	
P4	0.16	0.23	0.23	0.23	0.23	0.18	0.11	0.11	0.11	0.11	0.11	
P5	0.23	0.25	0.14	0.14	0.14	0.10	0.10	0.19	0.19	0.19	0.11	
P6	0.12	0.25	0.11	0.11	0.11	0.47	0.15	0.15	0.15	0.15	0.28	
P7	0.27	0.13	0.11	0.11	0.11	0.15	0.15	0.19	0.19	0.19	0.23	
P8	0.16	0.16	0.11	0.11	0.13	0.13	0.13	0.09	0.09	0.09	0.12	
P9	0.14	0.08	0.21	0.17	0.11	0.11	0.11	0.07	0.07	0.07	0.11	
P10	0.14	0.20	0.17	0.20	0.12	0.20	0.12	0.12	0.12	0.12	0.15	
Group	0.25	0.27	0.27	0.27	0.19	0.19	0.18	0.18	0.18	0.18	0.12	


Participant	(d) Sagittal											
	Lumbar						Upper thoracic					
	S1			S2			S1			S2		
	AvgSD	SI	S2	AvgSD	SI	S2	AvgSD	SI	S2	AvgSD	SI	S2
P1	0.13	0.23	0.18	0.23	0.23	0.18	0.20	0.11				
P2	0.38	0.25	0.27	0.35	0.20	0.20	0.20	0.13				
P3	0.24	0.19	0.18	0.16	0.08	0.08	0.08	0.23				
P4	0.23	0.27	0.27	0.30	0.22	0.22	0.22	0.15				
P5	0.26	0.24	0.13	0.28	0.20	0.20	0.20	0.26				
P6	0.21	0.26	0.29	0.29	0.17	0.17	0.17	0.17				
P7	0.38	0.17	0.55	0.51	0.09	0.09	0.09	0.22				
P8	0.12	0.17	0.19	0.18	0.06	0.06	0.06	0.06				
P9	0.34	0.16	0.29	0.24	0.23	0.23	0.23	0.17				
P10	0.23	0.24	0.18	0.26	0.24	0.24	0.24	0.36				
Group	0.16	0.24	0.26	0.23	0.15	0.15	0.15	0.09				

Participant	(e) Frontal											
	Lumbar						Upper thoracic					
	S1			S2			S1			S2		
	AvgSD	SI	S2	AvgSD	SI	S2	AvgSD	SI	S2	AvgSD	SI	S2
P1	0.55	0.38	0.12	0.12	0.13	0.07	0.15	0.12	0.12	0.12	0.15	
P2	0.22	0.17	0.13	0.11	0.18	0.18	0.18	0.11	0.18	0.16	0.15	
P3	0.10	0.17	0.11	0.23	0.23	0.18	0.11	0.11	0.08	0.08	0.19	
P4	0.16	0.23	0.23	0.23	0.23	0.18	0.11	0.11	0.11	0.11	0.11	
P5	0.23	0.25	0.14	0.14	0.14	0.10	0.10	0.19	0.19	0.19	0.11	
P6	0.12	0.25	0.11	0.11	0.11	0.47	0.15	0.15	0.15	0.15	0.28	
P7	0.27	0.13	0.11	0.11	0.11	0.15	0.15	0.19	0.19	0.19	0.23	
P8	0.16	0.16	0.11	0.11	0.13	0.13	0.13	0.09	0.09	0.09	0.12	
P9	0.14	0.08	0.21	0.17	0.11	0.11	0.11	0.07	0.07	0.07	0.11	
P10	0.14	0.20	0.17	0.20	0.12	0.20	0.12	0.12	0.12	0.12	0.15	
Group	0.25	0.27	0.27	0.27	0.19	0.19	0.18	0.18	0.18	0.18	0.12	

**Table 2. (Continued)**

Participant	(c) Transverse												(f) Transverse								
	Lumbar				Lower thoracic				Upper thoracic				Lumbar		Lower thoracic		Upper thoracic				
	S1	S2	Mean	SD	S1	S2	Mean	SD	S1	S2	Mean	SD	S1	S2	AvgSD	SI	S2	AvgSD	SI	S2	AvgSD
P1	9.23	1.03	9.50	0.40	7.52	0.52	7.92	0.52	18.91	2.89	16.06	1.17	0.26	0.21	0.40	0.30	0.63	0.32			
P2	8.41	0.72	8.66	1.18	5.99	1.46	5.98	0.85	15.67	2.24	14.11	1.51	0.27	0.21	0.31	0.28	0.54	0.33			
P3	6.28	0.30	5.05	0.79	5.21	0.86	5.71	0.53	7.43	0.86	7.07	0.90	0.17	0.27	0.17	0.33	0.14	0.26			
P4	7.13	1.05	6.85	0.33	5.37	0.74	3.85	0.53	16.04	2.42	11.94	1.16	0.46	0.19	0.34	0.18	0.87	0.31			
P5	12.59	1.04	13.11	0.98	6.20	1.19	6.17	1.07	8.99	1.08	10.75	1.95	0.88	0.41	0.71	0.25	0.38	0.41			
P6	8.15	0.77	7.75	2.05	7.28	1.09	6.37	1.56	13.76	0.92	12.19	1.08	0.29	0.20	0.20	0.19	0.25	0.26			
P7	7.28	0.40	7.71	1.72	4.12	0.54	3.83	0.75	9.05	1.00	9.46	0.90	0.24	0.24	0.19	0.23	0.43	0.29			
P8	6.42	0.34	6.52	0.41	3.38	1.23	4.27	1.01	4.28	0.34	5.74	1.15	0.26	0.17	0.24	0.16	0.22	0.18			
P9	6.66	1.16	7.41	1.28	6.82	1.05	7.56	2.06	7.30	1.28	7.72	1.34	0.31	0.35	0.23	0.30	0.27	0.43			
P10	5.73	0.56	9.87	0.60	3.12	0.40	4.81	0.82	11.98	1.28	12.68	1.70	0.15	0.28	0.20	0.21	0.28	0.43			
Group	7.79	2.00	8.24	2.22	5.50	1.56	5.65	1.45	11.34	4.68	10.77	3.27	0.52	0.45	0.34	0.38	0.74	0.41			

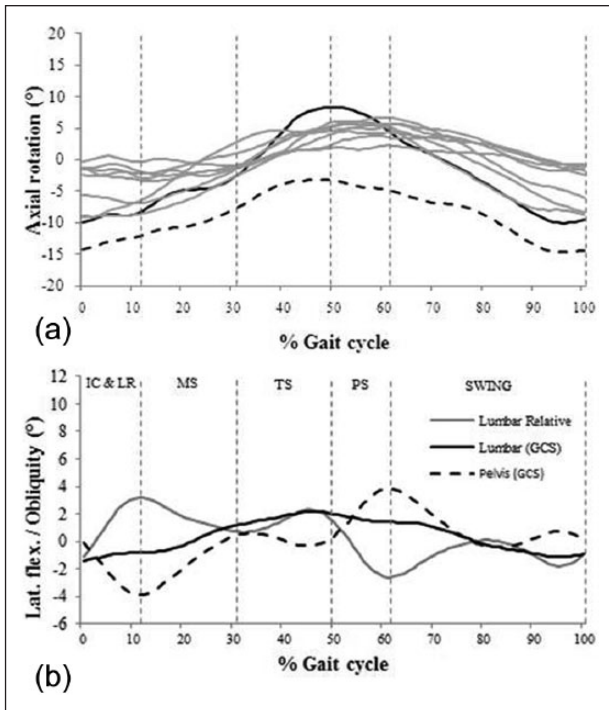

**Figure 5.** (a) Mean relative UT kinematic waveforms from 10 participants during gait and (b) pelvis and lumbar motion (relative and global) during gait in the frontal plane.

laboratory. However, external research is required to support the application of the 3D cluster technique in clinical practice.

While knowledge of relative movement between segments is important, understanding global kinematic waveforms assists in the explanation of relative data, provides valuable information about segmental dominance, can assess reproducibility of methodological procedures and allows for a detailed comparison between investigational findings. For instance, in the frontal plane (Figure 5(b)), peak pelvis downward obliquity coincided with peak relative lumbar lateral flexion to the right at approximately 12% of the gait cycle following toe off on the contra-lateral leg, a finding that is in agreement with previous investigations.<sup>15,20,40</sup> Subsequently, the pelvis dropped down on the contra-lateral side, while relative motion of the lumbar segment exhibited a lateral flexion towards the weight bearing limb. However, it is evident in this study that the lumbar segment was laterally flexed towards the left in reference to the GCS, which further reveals the dominance and contribution of the pelvis to relative motion. In contrast, Crosbie et al.<sup>15</sup> found the lumbar segment to be the main determinant of relative motion in comparison to the pelvis, and despite the fact that authors provided relative motion and a ROM value,

**Table 3.** Lumbar range of motion data from this study and published literature.

Study	Sagittal			Frontal			Transverse		
	Difference (+/-)			Difference (+/-)			Difference (+/-)		
	S1	S2		S1	S2		S1	S2	
3D cluster (L3)									
This study (S1)	3.22			6.50			7.79		
This study (S2)	3.03			6.63			8.24		
Konz et al. <sup>5</sup>	4.10	0.88	1.07	5.70	-0.80	-0.93	9.80	2.01	1.56
3D cluster (T12/L1)									
Thurston et al. <sup>19</sup>	5.10	1.88	2.07	9.30	2.80	2.67	8.30	0.51	0.06
Thurston <sup>33</sup>	7.10	3.88	4.07	8.70	2.20	2.07	6.00	-1.79	-2.24
Thurston and Harris <sup>20</sup>	5.20	1.98	2.17	8.50	2.00	1.87	8.30	0.51	0.06
Thurston <sup>34</sup>	5.20	1.98	2.17	6.80	0.30	0.17	8.80	1.01	0.56
Taylor et al. <sup>35</sup>	3.24	0.02	0.21	12.84	6.34	6.21	6.44	-1.35	-1.80
Taylor et al. <sup>36</sup>	3.83	0.61	0.80	11.98	5.48	5.35	6.39	-1.40	-1.85
Taylor et al. <sup>21</sup>	3.40	0.18	0.37	10.20	3.70	3.57	6.20	-1.59	-2.04
Taylor et al. <sup>22</sup>	3.00	-0.22	-0.03	9.20	2.70	2.57	6.20	-1.59	-2.04
Vogt and Banzer <sup>17</sup>	2.40	-0.82	-0.63	2.80	-3.70	-3.83	6.80	-0.99	-1.44
Vogt et al. <sup>37</sup>	2.40	-0.82	-0.63	2.84	-3.66	-3.79	6.80	-0.99	-1.44
Vogt et al. <sup>38</sup>	4.10	0.88	1.07	2.80	-3.70	-3.83	8.60	0.81	0.36
Callaghan et al. <sup>39</sup>	7.53	4.31	4.50	6.01	-0.49	-0.62	11.18	3.39	2.94
Whittle and Levine <sup>40</sup>	3.98	0.76	0.95	7.55	1.05	0.92	8.34	0.55	0.10
Morgenroth et al. <sup>23</sup>	5.10	1.88	2.07	5.30	-1.20	-1.33	11.30	3.51	3.06
Bone pins									
MacWilliams et al. <sup>32</sup>									
L1 relative to pelvis	3.00	-0.22	-0.03	10.40	3.90	3.77	4.50	-3.29	-3.74
L3 relative to pelvis	2.30	-0.92	-0.73	6.50	0.00	-0.13	3.50	-4.29	-4.74

global frontal plane movement for the lumbar segment was not considered so further interpretation was not possible. In this study, lateral flexion towards the weight bearing limb did not take place until approximately half way through MS. Relative lumbar segment movement underwent a lateral flexion to the right during TS. While this finding is in agreement with Whittle and Levine,<sup>40</sup> the authors provided no reason for the additional relative lateral flexion towards the weight bearing limb at this stage of the gait cycle. It can be clearly seen in this study, the lumbar segment in reference to the GCS continues to flex laterally to the right at the start of TS, with peak relative lumbar movement corresponding to peak movement in reference to the GCS, and the reason for the second peak in right lateral lumbar flexion. [AQ: 8]

The results of this study were based on the application of 3D clusters by one examiner; therefore, a future investigation involving multiple examiners is needed to further examine the reliability of the proposed marker configuration. In addition to this, the effect of the plate and its relationship to the back could be investigated. However, while it is accepted that pelvis and lumbar global angular data could have been influenced by soft tissue artefact, ROM values presented in Table 2 are consistent with those previously reported.<sup>5</sup> Finally, the angular kinematic data in this study was collected from a small sample size, so additional participants are required to confirm the findings of this study along with the analysis of female and clinical populations.

## Conclusion

This study proposed validity and reliability measures of a new kinematic model developed to assess regional movement of the spine using a 3D cluster technique. The applied marker configuration demonstrated inter-segmental movement of the thoracic spine, suggesting that this region of the spine should not be modelled as a single rigid segment. 3D movement analysis of the lumbar movement compared well to previously published data; however, supportive evidence is lacking as previous investigations provide only ROM values or relative kinematic waveforms and ROM. Conversely, as shown in the findings of this study, global movements provide valuable information on the interpretation of relative angle data.

## Author contribution

All the authors contributed equally in the preparation of this manuscript. [AQ: 9]

## Declaration of conflicting interests

The authors report no conflict of interest.

## Funding

This research received no specific grant from any funding agency in the public, commercial or not-for-profit sectors.

## References

1. Kakushima M, Miyamoto K and Shimizu K. The effect of leg length discrepancy on spinal motion during gait: three-dimensional analysis in healthy volunteers. *Spine* 2003; 28(21): 2472–2476. [AQ: 10]
2. Newman N, Gracovetsky S, Itoi M, et al. Can the computerized physical examination differentiate normal subjects from abnormal subjects with benign mechanical low back pain? *Clin Biomech* 1996; 11(8): 466–473.
3. Gracovetsky SA. Range of normality versus range of motion: a functional measure for the prevention and management of low back injury. *J Bodyw Mov Ther* 2010; 14(1): 40–49.
4. Chockalingam N, Dangerfield PH, Giakas G, et al. Study of marker placements in the back for opto-electronic motion analysis. *Stud Health Technol Inform* 2002; 88: 105–109.
5. Konz RJ, Fatone S, Stine RL, et al. A kinematic model to assess spinal motion during walking. *Spine* 2006; 31(24): E898–E906.
6. Stebbins J, Harrington M, Thompson N, et al. Repeatability of a model for measuring multi-segment foot kinematics in children. *Gait Posture* 2006; 23(4): 401–410.
7. Manal K, McClay I, Stanhope S, et al. Comparison of surface mounted markers and attachment methods in estimating tibial rotations during walking: an in vivo study. *Gait Posture* 2000; 11(1): 38–45.
8. Chockalingam N, Chevalier TL, Young MK, et al. Marker placement for movement analysis in scoliotic patients: a critical analysis of existing systems. *Stud Health Technol Inform* 2008; 140: 166–169.
9. Frigo C, Carabalona R, Dalla Mura M, et al. The upper body segmental movements during walking by young females. *Clin Biomech* 2003; 18(5): 419–425.
10. Rowe PJ and White M. Three dimensional, lumbar spinal kinematics during gait, following mild musculo-skeletal low back pain in nurses. *Gait Posture* 1996; 4(3): 242–251.
11. Leardini A, Biagi F, Merlo A, et al. Multi-segment trunk kinematics during locomotion and elementary exercises. *Clin Biomech* 2011; 26(6): 562–571.
12. Armand S, Sangeux M and Baker R. Optimal markers' placement on the thorax for clinical gait analysis. *Gait Posture* 2014; 39(1): 147–153.
13. Thummerer Y, von Kries R, Marton M-A, et al. Is age or speed the predominant factor in the development of trunk movement in normally developing children? *Gait Posture* 2012; 35(1): 23–28.
14. Wu G, van der Helm FC, Veeger HEJ, et al. ISB recommendation on definitions of joint coordinate systems of various joints for the reporting of human joint motion – part II: shoulder, elbow, wrist and hand. *J Biomech* 2005; 38(5): 981–992.
15. Crosbie J, Vachalathiti R and Smith R. Patterns of spinal motion during walking. *Gait Posture* 1997; 5(1): 6–12.
16. Syczewska M, Oberg T and Karlsson D. Segmental movements of the spine during treadmill walking with normal speed. *Clin Biomech* 1999; 14(6): 384–388.
17. Vogt L and Banzer W. Measurement of lumbar spine kinematics in incline treadmill walking. *Gait Posture* 1999; 9(1): 18–23.

18. Pearcy MJ, Gill JM, Whittle MW, et al. Dynamic back movement measured using a three-dimensional television system. *J Biomech* 1987; 20(10): 943–949.
19. Thurston AJ, Whittle MW and Stokes IAF. Spinal and pelvic movement during walking – a new method of study. *Arch Eng Med 1971–1988 (vols 1–17)* 1981; 10(4): 219–222.
20. Thurston AJ and Harris JD. Normal kinematics of the lumbar spine and pelvis. *Spine* 1983; 8(2): 199–205.
21. Taylor NF, Evans OM and Goldie PA. The effect of walking faster on people with acute low back pain. *Eur Spine J* 2003; 12(2): 166–172.
22. Taylor N, Goldie P and Evans O. Movements of the pelvis and lumbar spine during walking in people with acute low back pain. *Physiother Res Int* 2004; 9(2): 74–84.
23. Morgenroth DC, Orendurff MS, Shakir A, et al. The relationship between lumbar spine kinematics during gait and low-back pain in transfemoral amputees. *Am J Phys Med Rehabil* 2010; 89(8): 635–643.
24. Rice J, Walsh M, Jenkinson A, et al. Measuring movement at the low back. *Clin Anat* 2002; 15(2): 88–92.
25. Whittle MW and Levine D. Measurement of lumbar lordosis as a component of clinical gait analysis. *Gait Posture* 1997; 5(2): 101–107.
26. Grood ES and Suntay WJ. A joint coordinate system for the clinical description of three-dimensional motions: application to the knee. *J Biomech Eng* 1983; 105(2): 136–144.
27. Winter DA, Sidwall HG and Hobson DA. Measurement and reduction of noise in kinematics of locomotion. *J Biomech* 1974; 7(2): 157–159.
28. Perriman DM, Scarvell JM, Hughes AR, et al. Validation of the flexible electrogoniometer for measuring thoracic kyphosis. *Spine* 2010; 35(14): E633–E640.
29. Perry J and Burnfield J. *Gait analysis: normal and pathological function*. 2nd ed. Thorofare, NJ: SLACK Incorporated, 2010.
30. Chockalingam N, Dangerfield PH, Rahmatalla A, et al. A comparison of three kinematic systems for assessing spinal range of movement. *Int J Ther Rehabil* 2003; 10(9): 402–407.
31. Pearcy MJ, Gill JM, Hindle RJ, et al. Measurement of human back movements in three dimensions by opto-electronic devices. *Clin Biomech* 1987; 2(4): 199–204.
32. MacWilliams BA, Rozumalski A, Swanson AN, et al. Assessment of three-dimensional lumbar spine vertebral motion during gait with use of indwelling bone pins. *J Bone Joint Surg Am* 2013; 95(23): e1841–e1848.
33. Thurston AJ. Repeatability studies of a television/computer system for measuring spinal and pelvic movements. *J Biomed Eng* 1982; 4(2): 129–132.
34. Thurston AJ. Spinal and pelvic kinematics in osteoarthritis of the hip joint. *Spine* 1985; 10(5): 467–471.
35. Taylor NF, Evans OM and Goldie PA. Angular movements of the lumbar spine and pelvis can be reliably measured after 4 minutes of treadmill walking. *Clin Biomech* 1996; 11(8): 484–486.
36. Taylor NF, Goldie PA and Evans OM. Angular movements of the pelvis and lumbar spine during self-selected and slow walking speeds. *Gait Posture* 1999; 9(2): 88–94.
37. Vogt L, Pfeifer K, Portscher M, et al. Influences of non-specific low back pain on three-dimensional lumbar spine kinematics in locomotion. *Spine* 2001; 26(17): 1910–1919.
38. Vogt L, Pfeifer K and Banzer W. Comparison of angular lumbar spine and pelvis kinematics during treadmill and overground locomotion. *Clin Biomech* 2002; 17(2): 162–165.
39. Callaghan JP, Patla AE and McGill SM. Low back three-dimensional joint forces, kinematics, and kinetics during walking. *Clin Biomech* 1999; 14(3): 203–216.
40. Whittle MW and Levine D. Three-dimensional relationships between the movements of the pelvis and lumbar spine during normal gait. *Hum Mov Sci* 1999; 18(5): 681–692.